

PCR Quantification with Melt Curve Report
PCR Base Line Subtracted Data
Graphs Only


Current Date: 11-Oct-06 12:48 PM
Data generated on: 19-Aug-05 at 02:23 PM.

Optical data file name: val 81905 #5.odm
Plate Setup file used: 6pt5fold8s_crs.psm
Protocol file used: Alison78DC.tmo

Sample volume: 20.00 ul
Hot Start? No
Well factor collection: Experimental Plate

Comments


PCR Amp/Cycle Graph for SYBR-490

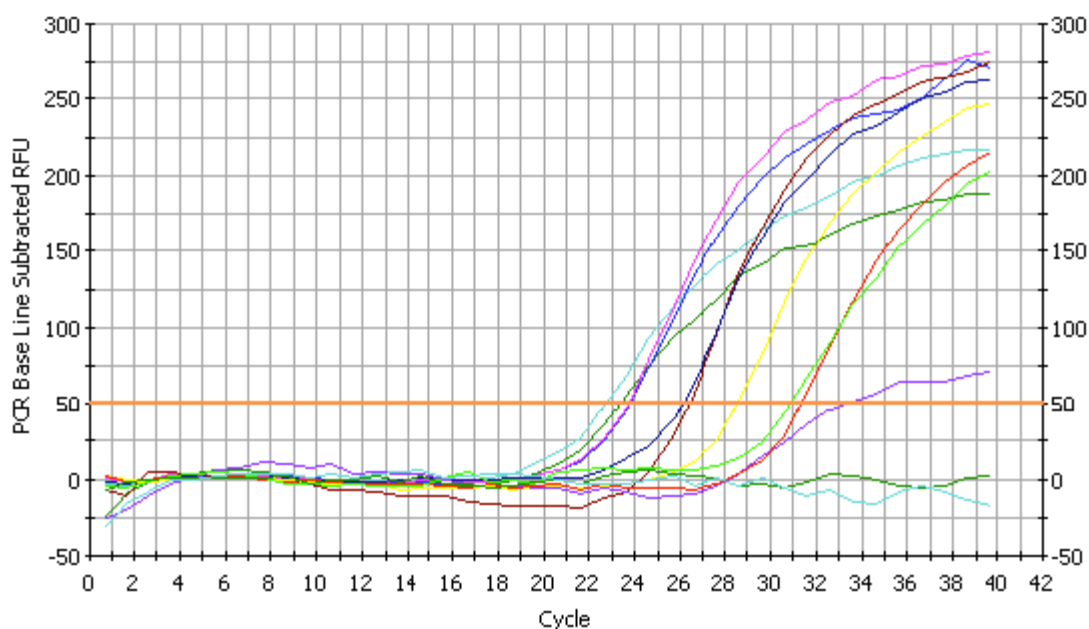

Data Analysis Parameters

Calculated threshold has been replaced by the user selected threshold **50.0**.
Per-well baseline cycles have been determined automatically.
Data analysis window is set at **95.00%** of a cycle, centered at **end** of the cycle.
Weighted Mean digital filtering has been applied. Global filtering is **off**.

Melt Curve Graph for SYBR-490

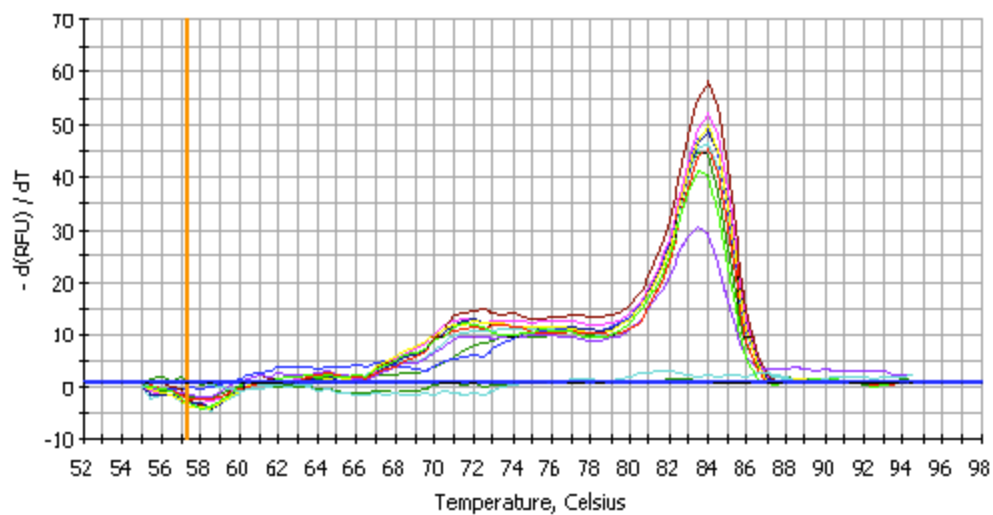

Melt Curve Analysis Parameters

Weighted Mean digital filtering has been applied. Global filtering is **off**.
Threshold for automatic peak detection is set at **1.00**.